

Central Lancashire Online Knowledge (CLoK)

Title	Evaluation of microFLOQ™ Direct Swab for Touch DNA Recovery
Type	Article
URL	https://clock.uclan.ac.uk/51190/
DOI	##doi##
Date	2024
Citation	Alketbi, Salem Khalifa orcid iconORCID: 0000-0002-7773-3953 and Goodwin, William H orcid iconORCID: 0000-0002-3632-3552 (2024) Evaluation of microFLOQ™ Direct Swab for Touch DNA Recovery. Journal of Forensic Legal & Investigative Sciences . ISSN 2473-733X
Creators	Alketbi, Salem Khalifa and Goodwin, William H

It is advisable to refer to the publisher's version if you intend to cite from the work. ##doi##

For information about Research at UCLan please go to <http://www.uclan.ac.uk/research/>

All outputs in CLoK are protected by Intellectual Property Rights law, including Copyright law. Copyright, IPR and Moral Rights for the works on this site are retained by the individual authors and/or other copyright owners. Terms and conditions for use of this material are defined in the <http://clock.uclan.ac.uk/policies/>

Research Article

Evaluation of microFLOQ™ Direct Swab for Touch DNA Recovery

Alketbi Salem K^{1,2*} and Goodwin W²

¹General Department of Forensic Science and Criminology, Dubai Police, Dubai, UAE

²University of Central Lancashire, Preston, UK

Abstract

This study evaluates the efficacy of the microFLOQ™ Direct Swab for touch DNA recovery from various surfaces within an office environment. Samples were collected using the swab and subjected to direct amplification with the GlobalFiler™ PCR Kit. Results revealed a success rate of 73% within three hours post-sample collection, with profiles ranging from full single to partial mixture. Despite observed artifacts, such as split and shoulder peaks, the swab demonstrated potential for efficient touch DNA recovery. However, further research is needed to assess its performance across diverse surfaces and to address challenges associated with artifact generation. Overall, the microFLOQ™ Direct Swab shows promise as a valuable tool for forensic touch DNA analysis, offering streamlined sample processing and potential advancements in forensic casework.

Keywords: Direct amplification; DNA profiling; Forensic science; Forensic investigation; GlobalFiler™ PCR Amplification Kit; MicroFLOQ™ Direct swabs; Touch DNA

Introduction

Trace or Touch DNA profiling plays a crucial role in linking individuals to criminal activities, often detected in minute quantities on various items found at crime scenes, setting it apart from other types of DNA evidence such as body fluids [1-3]. However, Touch DNA poses several challenges, including the risk of cross-contamination at crime scenes [4]. Factors such as surface types, collection methods, and environmental conditions influence the amount of Touch DNA retrieved, thereby complicating analysis [5-9]. Moreover, the extraction process and purification steps currently employed in forensic DNA

*Corresponding author: Alketbi Salem K, General Department of Forensic Science and Criminology, Dubai Police, Dubai, UAE and University of Central Lancashire, Preston, UK, Tel: 00447774141205; Email: alkitbe.11@hotmail.com

Citation: Alketbi SK, Goodwin W (2024) Evaluation of microFLOQ™ Direct Swab for Touch DNA Recovery. *Forensic Leg Investig Sci* 10: 093.

Received: March 19, 2023; **Accepted:** March 28, 2024; **Published:** April 05, 2024

Copyright: © 2024 Alketbi SK, et al. This is an open-access article distributed under the terms of the Creative Commons Attribution License, which permits unrestricted use, distribution, and reproduction in any medium, provided the original author and source are credited.

casework are time-consuming and labor-intensive. Column-based purification methods can lead to DNA loss, potentially impacting the successful typing of degraded or low-copy-number samples [10-15]. Efforts to validate different collection techniques with varied methods can enhance Touch DNA recovery from a variety of surfaces [16-20].

Direct amplification in DNA profiling eliminates the need for DNA extraction and quantification, proceeding directly to PCR after sample collection. This approach not only improves recovery but also reduces the risk of errors, minimizes contamination from handling, and decreases both processing time and associated costs [1]. Recent interest has focused on developing innovative protocols for direct amplification; however, there remains limited shared knowledge regarding trace DNA collection techniques for direct PCR from casework samples [21]. One promising approach involves the use of the microFLOQ® Direct swab, a product co-developed by the French Gendarmerie Forensic Research Institute (IRCGN™) and Copan, which has shown effectiveness in collecting trace DNA for direct amplification [22-25]. The microFLOQ® Direct swabs are designed similarly to 4N6 FLOQswabs® but are treated with a lysing agent for direct amplification, eliminating the need for DNA extraction and quantification [26]. Utilization of these swabs allows for DNA profiling from sample collection to final result in less than two hours. Additionally, due to the small dimensions of the microFLOQ® swab head, only a minimal portion of a stain is collected, resulting in significantly reduced sample consumption compared to traditional swabbing methods. Efforts to reduce sample consumption enable more evidence to be retained for retesting or post-conviction testing, if desired. Therefore, the aim of this study was to investigate the effectiveness of microFLOQ™ Direct swabs in recovering touch DNA from random surfaces of office items to replicate casework samples.

Materials and Methods

Touch samples

Biological materials were collected from a varied selection of surfaces commonly encountered in an office environment. To mimic the workflow of actual casework, these surfaces were randomly chosen, and the duration of DNA deposition was unspecified; some surfaces were routinely touched by users on a daily basis, while others had not been touched for an extended period. The sampled surfaces comprised three computer mice, three computer keyboards, two door handles, two window handles, two pens, an old handprint on a window, a leather wallet, and a cell phone (refer to Figure 1).

DNA recovery

The MicroFLOQ Direct swabs were employed to retrieve trace DNA from the surfaces outlined in Figure 1. Prior to sampling, each MicroFLOQ® Direct swab was moistened with 1µl of molecular-grade water using a pipette, following the manufacturer's instructions. Subsequently, the swab head was gently rubbed and rotated across the surface in a subsampling fashion to collect the sample.









Items	quantity
 Computer mouse (CM)	3
 Computer keyboard (CK)	3
 Door handle (DH)	2
 Window handle (WH)	2
 Pen (PN)	2
 Handprint on a window (HP)	1
 Leather wallet (LW)	1
 Cell phone (CP)	1

Figure 1: Office Items Utilized for Touch DNA collection to be processed for direct amplification.

Direct PCR amplification

Following sample collection, the tips of the MicroFLOQ® Direct swabs were detached into PCR strip tubes (0.2 ml) and subjected to amplification using the GlobalFiler™ amplification Kit (Thermo Fisher Scientific) [27], adhering to Copan’s Direct DNA Analysis protocol with the microFLOQ® Collection Device [22]. This protocol involved substituting the volume of sample solution required by the kit manufacturer with molecular-grade water (15 µL), directly adding PCR master mix to the tubes (10 µL), and conducting immediate amplification on an ABI GeneAmp® 9700 PCR System (Life Technologies) for 29 cycles, following the manufacturer’s recommended conditions. To evaluate potential inhibition from the lysing agent incorporated into the swab head fibers, positive control DNA (007) was amplified in the presence of a MicroFLOQ® Direct swab. Additionally, negative controls consisting solely of the MicroFLOQ® swab head were included.



DNA detection, separation, and analysis

The amplified products underwent size separation and detection on an ABI 3500 Genetic Analyzer (Life Technologies) using a mixture comprising 1 µl of PCR product, 9.6 µl of Hi-Di™ formamide, and 0.4 µl of GeneScan™ 600 LIZ® Size Standard v2.0 (Thermo Fisher Scientific). At least one microliter of allelic ladder was included per injection on the 96-well plate. Following denaturation at 95°C for 5 minutes, samples were promptly cooled on ice for 5 minutes. Electrophoresis was conducted on a 36-cm capillary array with POP-4™ polymer (Life Technologies) using standard injection parameters (1.2 kV, 24 s). Subsequently, STR data were sized and typed utilizing GeneMapper® ID-X Software Version 1.2 (Life Technologies), employing manufacturer-validated analytical thresholds.

Results and Discussion

The utilization of MicroFLOQ® swabs with the GlobalFiler™ amplification Kit for direct PCR, aimed at recovering Touch DNA

from assorted items within an office setting, yielded a success rate of 73% within a three-hour timeframe post-sample collection. Out of the 15 samples collected, 11 STR profiles yielded positive DNA results suitable for database search. These profiles comprised full single, partial single, full mixture, and partial mixture DNA profiles (refer to Figures 2&3). However, the majority of profiles exhibited artifacts such as split and shoulder peaks. As per the criteria set by the Biology and DNA Section lab within the General Department of Forensic Science and Criminology, positive DNA results for forensic trace profiles necessitate homozygous or heterozygous alleles, or a combination thereof, in a minimum of nine loci. The negative control employed in the DNA profiling process was confirmed to be free of DNA. Additionally, amplification of Positive control DNA (007) in the presence of a MicroFLOQ® swab head resulted in complete STR profiles, demonstrating expected performance. This outcome suggests that the chemical treatment of MicroFLOQ® swab heads with a lysing agent by the manufacturer does not impede or inhibit successful DNA amplification.

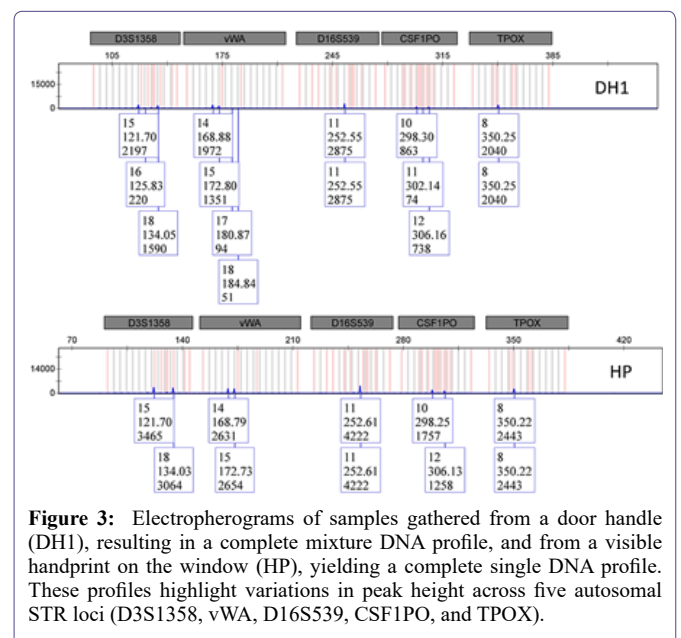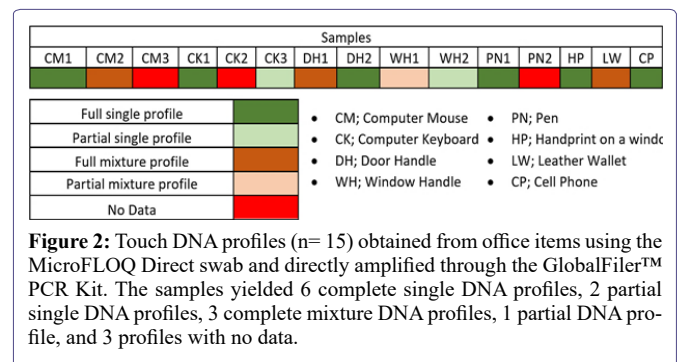

Previous research by Templeton et al. [28] compared the performance of foam swabs, cotton swabs, and nylon FLOQSwabs® in collecting trace DNA from fingerprints, with the latter demonstrating the highest DNA yield. This study was expanded to include the use of FLOQSwabs® for touch DNA recovery across various substrates, comparing direct amplification to the standard extraction workflow.

Findings from these controlled experiments underscore the potential of the FLOQSwab® system and direct amplification in enhancing signal retrieval from low-level touch samples, while conserving resources and mitigating contamination risks [29].

Moreover, the adoption of direct detection facilitated a rapid DNA profiling process, albeit accompanied by the observation of artifacts such as split and shoulder peaks, consistent with prior reports [23-24]. Distinguishing true alleles within DNA profiles can be straightforward when originating from a single source, yet becomes complex in mixed DNA profiles, particularly in the absence of reference samples.

The results obtained from this limited set of touch samples suggest that the miniaturized microFLOQ® swab head can retrieve sufficient cellular material to generate complete DNA profiles from diverse surfaces. However, the quantity of material present and the nature of the surface influence the likelihood of success, as anticipated for evidence collection via swabbing.

Conclusion

In conclusion, the findings of this study provide valuable insights into the effectiveness of the MicroFLOQ™ Direct Swab for Touch DNA recovery. While the results demonstrate promising success rates within a controlled office environment, further research is necessary to comprehensively evaluate its efficiency across a broader spectrum of surfaces and scenarios. Additionally, the observed artifacts, such as split and shoulder peaks, underscore the need for future work to develop strategies to mitigate these challenges associated with direct amplification. By addressing these areas of improvement, the MicroFLOQ™ Direct Swab has the potential to become an invaluable tool in forensic investigations, offering enhanced efficiency and reliability in Touch DNA recovery.

Conflict of interest

None.

Acknowledgement

The authors would like to express their gratitude to the General Department of Forensic Science and Criminology in Dubai Police for approving this study. Ethical approval was granted by the University of Central Lancashire's Research Ethics Committee (ref. no. STEMH 912), for which we are sincerely thankful.

References

- Alketbi SK (2018) The affecting factors of Touch DNA. *J of Forensic Res* 9: 424.
- Alketbi SK (2023) Analysis of Touch DNA. Doctoral thesis, University of Central Lancashire.
- Alketbi, SK (2023) The role of DNA in forensic science: A comprehensive review. *Int J of Sci and Res Arch* 9: 814-829.
- Alketbi SK (2023) Maintaining the chain of custody: Anti-contamination measures for trace DNA evidence. *International J Sci Res Arch* 8: 457-461.
- Alketbi SK, Goodwin W (2019) The effect of surface type, collection, and extraction methods on Touch DNA. *Forensic Science International. Genetics Supplement Series* 7: 704-706.
- Alketbi SK, Goodwin W (2019) The effect of time and environmental conditions on Touch DNA. *Forensic Science International. Genetics Supplement Series* 7: 701-703.
- Alketbi SK, Goodwin W (2019) The effect of sandy surfaces on Touch DNA. *Journal of Forensic Legal & Investigative Sciences* 5: 034.
- Alketbi SK (2020) Collection of Touch DNA from rotten banana skin. *International Journal of Forensic Sciences* 5: 000204.
- Alketbi SK (2023) An Evaluation of the Performance of Two Quantification Methods for Trace DNA Casework Samples. *J Forensic Sci Criminal Invest* 16: 555950.
- Barta JL, Monroe C, Teisberg JE, Winters M, Kemp BM, et al. (2014) One of the key characteristics of ancient DNA, low copy number, may be a product of its extraction. *J of archaeol sci* 46: 281-289.
- Mumy KL, Findlay RH (2004) Convenient determination of DNA extraction efficiency using an external DNA recovery standard and quantitative-competitive PCR. *J microbiol methods* 57: 259-268.
- Dabney J, Knapp M, Gansauge MT, Weihmann A, Nickel B, et al. (2013) Complete mitochondrial genome sequence of a Middle Pleistocene cave bear reconstructed from ultrashort DNA fragments. *Proceedings of the National Academy of Sciences - PNAS* 110: 15758-15763.
- Kemp BM, Winters M, Monroe C, Barta JL (2014) How Much DNA is Lost? Measuring DNA Loss of Short-Tandem-Repeat Length Fragments Targeted by the PowerPlex 16® System Using the Qiagen MinElute Purification Kit. *Human biology* 86: 313-329.
- Doran AE, Foran DR (2014) Assessment and mitigation of DNA loss utilizing centrifugal filtration devices. *Forensic science international: Genetics* 13: 187-190.
- Garvin AM, Fritsch A (2013) Purifying and Concentrating Genomic DNA from Mock Forensic Samples Using Millipore Amicon Filters. *Journal of forensic sciences* 58: S173-S175.
- Alketbi SK, Goodwin W (2021) Touch DNA collection techniques for non-porous surfaces using cotton and nylon swabs. *Biomedical Journal of Scientific & Technical Research* 36: 28608-28612.
- Alketbi SK (2022) The impact of collection method on Touch DNA collected from fabric. *Journal of Forensic Sciences and Criminal Investigation* 15: 555922.
- Alketbi SK, Goodwin W (2022) The impact of area size and fabric type on Touch DNA collected from fabric. *Journal of Forensic Sciences and Criminal Investigation* 16: 555926.
- Alketbi SK, Goodwin W (2022) The impact of deposition area and time on Touch DNA collected from fabric. *Forensic Science International, Genetics Supplement Series* 8: 45-47.
- Alketbi SK (2023) Collection techniques of touch DNA deposited on human skin following a strangulation scenario. *International Journal of Legal Medicine* 137: 1347-1352 .
- Cavanaugh SE, Bathrick AS (2018) Direct PCR amplification of forensic touch and other challenging DNA samples: A review. *Forensic science international: Genetics* 32: 40-49.
- Ambers A, Wiley R, Novroski N, Budowle B (2018) Direct PCR amplification of DNA from human bloodstains, saliva, and touch samples collected with microFLOQ® swabs. *Forensic science international: Genetics* 32: 80-87.
- Alketbi SK, Goodwin W (2023) Collection Methods for Touch DNA Direct Amplification. *Journal of Forensic, Legal and Investigative Sciences* 9: 072.
- Alketbi SK (2022) An innovative solution to collect Touch DNA for direct amplification. *Journal of Forensic Sciences and Criminal Investigation* 16: 555928.
- Alketbi SK, Alsoofi S (2022) Dual recovery of DNA and fingerprints using Minitapes. *Journal of Forensic Sciences and Criminal Investigation* 16: 555929.

26. microFLOQ® Direct product brochure, <https://www.copangroup.com/product-ranges/microfloq/>
27. GlobalFiler™ PCR amplification kit user guide. (2016) Revision E.
28. Templeton J, Blackie R, Viviana P, Oliva H, Taylor D (2013) Genetic profiling from challenging samples: Direct PCR of touch DNA. *Forensic science international. Genetics supplement series 4*: e224-e225.
29. Templeton JE, Taylor D, Handt O, Skuza P, Linacre A (2015) Direct PCR Improves the Recovery of DNA from Various Substrates. *Journal of forensic sciences* 60: 1558-1562.



- Advances In Industrial Biotechnology | ISSN: 2639-5665
- Advances In Microbiology Research | ISSN: 2689-694X
- Archives Of Surgery And Surgical Education | ISSN: 2689-3126
- Archives Of Urology
- Archives Of Zoological Studies | ISSN: 2640-7779
- Current Trends Medical And Biological Engineering
- International Journal Of Case Reports And Therapeutic Studies | ISSN: 2689-310X
- Journal Of Addiction & Addictive Disorders | ISSN: 2578-7276
- Journal Of Agronomy & Agricultural Science | ISSN: 2689-8292
- Journal Of AIDS Clinical Research & STDs | ISSN: 2572-7370
- Journal Of Alcoholism Drug Abuse & Substance Dependence | ISSN: 2572-9594
- Journal Of Allergy Disorders & Therapy | ISSN: 2470-749X
- Journal Of Alternative Complementary & Integrative Medicine | ISSN: 2470-7562
- Journal Of Alzheimers & Neurodegenerative Diseases | ISSN: 2572-9608
- Journal Of Anesthesia & Clinical Care | ISSN: 2378-8879
- Journal Of Angiology & Vascular Surgery | ISSN: 2572-7397
- Journal Of Animal Research & Veterinary Science | ISSN: 2639-3751
- Journal Of Aquaculture & Fisheries | ISSN: 2576-5523
- Journal Of Atmospheric & Earth Sciences | ISSN: 2689-8780
- Journal Of Biotech Research & Biochemistry
- Journal Of Brain & Neuroscience Research
- Journal Of Cancer Biology & Treatment | ISSN: 2470-7546
- Journal Of Cardiology Study & Research | ISSN: 2640-768X
- Journal Of Cell Biology & Cell Metabolism | ISSN: 2381-1943
- Journal Of Clinical Dermatology & Therapy | ISSN: 2378-8771
- Journal Of Clinical Immunology & Immunotherapy | ISSN: 2378-8844
- Journal Of Clinical Studies & Medical Case Reports | ISSN: 2378-8801
- Journal Of Community Medicine & Public Health Care | ISSN: 2381-1978
- Journal Of Cytology & Tissue Biology | ISSN: 2378-9107
- Journal Of Dairy Research & Technology | ISSN: 2688-9315
- Journal Of Dentistry Oral Health & Cosmesis | ISSN: 2473-6783
- Journal Of Diabetes & Metabolic Disorders | ISSN: 2381-201X
- Journal Of Emergency Medicine Trauma & Surgical Care | ISSN: 2378-8798
- Journal Of Environmental Science Current Research | ISSN: 2643-5020
- Journal Of Food Science & Nutrition | ISSN: 2470-1076
- Journal Of Forensic Legal & Investigative Sciences | ISSN: 2473-733X
- Journal Of Gastroenterology & Hepatology Research | ISSN: 2574-2566
- Journal Of Genetics & Genomic Sciences | ISSN: 2574-2485
- Journal Of Gerontology & Geriatric Medicine | ISSN: 2381-8662
- Journal Of Hematology Blood Transfusion & Disorders | ISSN: 2572-2999
- Journal Of Hospice & Palliative Medical Care
- Journal Of Human Endocrinology | ISSN: 2572-9640
- Journal Of Infectious & Non Infectious Diseases | ISSN: 2381-8654
- Journal Of Internal Medicine & Primary Healthcare | ISSN: 2574-2493
- Journal Of Light & Laser Current Trends
- Journal Of Medicine Study & Research | ISSN: 2639-5657
- Journal Of Modern Chemical Sciences
- Journal Of Nanotechnology Nanomedicine & Nanobiotechnology | ISSN: 2381-2044
- Journal Of Neonatology & Clinical Pediatrics | ISSN: 2378-878X
- Journal Of Nephrology & Renal Therapy | ISSN: 2473-7313
- Journal Of Non Invasive Vascular Investigation | ISSN: 2572-7400
- Journal Of Nuclear Medicine Radiology & Radiation Therapy | ISSN: 2572-7419
- Journal Of Obesity & Weight Loss | ISSN: 2473-7372
- Journal Of Ophthalmology & Clinical Research | ISSN: 2378-8887
- Journal Of Orthopedic Research & Physiotherapy | ISSN: 2381-2052
- Journal Of Otolaryngology Head & Neck Surgery | ISSN: 2573-010X
- Journal Of Pathology Clinical & Medical Research
- Journal Of Pharmacology Pharmaceutics & Pharmacovigilance | ISSN: 2639-5649
- Journal Of Physical Medicine Rehabilitation & Disabilities | ISSN: 2381-8670
- Journal Of Plant Science Current Research | ISSN: 2639-3743
- Journal Of Practical & Professional Nursing | ISSN: 2639-5681
- Journal Of Protein Research & Bioinformatics
- Journal Of Psychiatry Depression & Anxiety | ISSN: 2573-0150
- Journal Of Pulmonary Medicine & Respiratory Research | ISSN: 2573-0177
- Journal Of Reproductive Medicine Gynaecology & Obstetrics | ISSN: 2574-2574
- Journal Of Stem Cells Research Development & Therapy | ISSN: 2381-2060
- Journal Of Surgery Current Trends & Innovations | ISSN: 2578-7284
- Journal Of Toxicology Current Research | ISSN: 2639-3735
- Journal Of Translational Science And Research
- Journal Of Vaccines Research & Vaccination | ISSN: 2573-0193
- Journal Of Virology & Antivirals
- Sports Medicine And Injury Care Journal | ISSN: 2689-8829
- Trends In Anatomy & Physiology | ISSN: 2640-7752

Submit Your Manuscript: <https://www.heraldopenaccess.us/submit-manuscript>